This Page Is Inserted by IFW Operations and is not a part of the Official Record

BEST AVAILABLE IMAGES


Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

As rescanning documents will not correct images, please do not report the images to the Image Problem Mailbox.



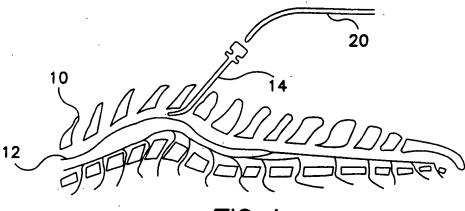
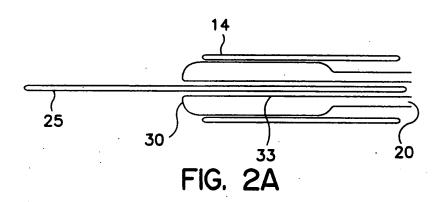


FIG. I







FIG. 2B




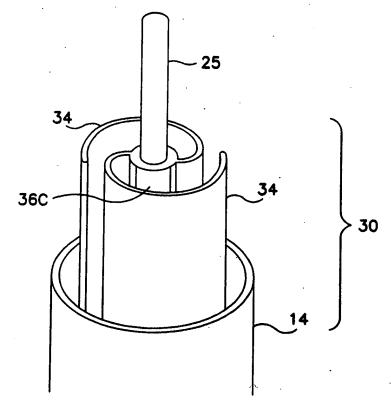


FIG. 2C

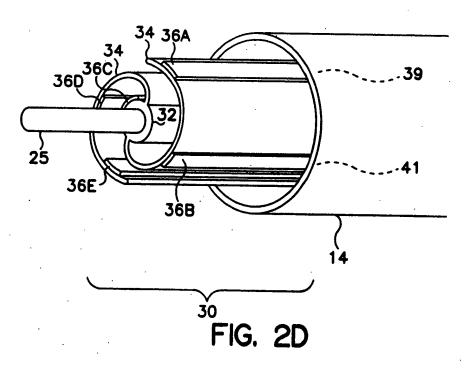

Banner & Witcoff, Ltd

Title: Apparatus and Method for Expanding A Stimulation Lead Body in Situ
Inventor: King et al.
Serial No.: (TBA)
Atty. Docket No. 11738.00215
Replacement Sheet Page 3 of 15

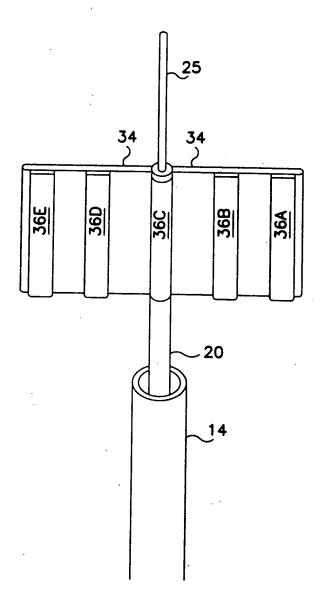


FIG. 2E

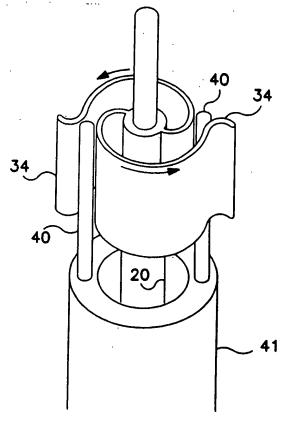


FIG. 3

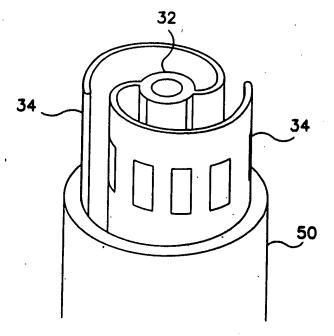



FIG. 4A



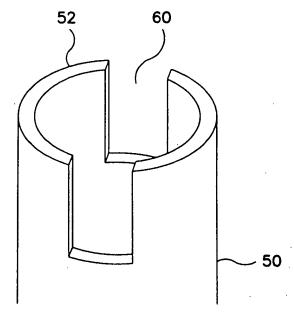


FIG. 4B

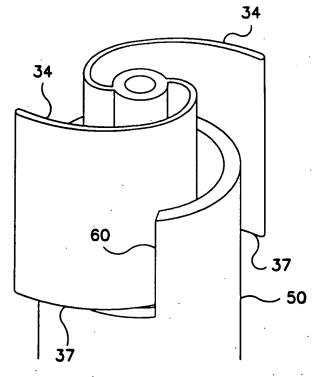
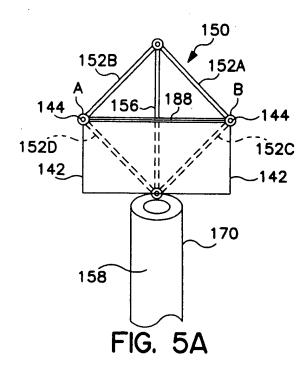
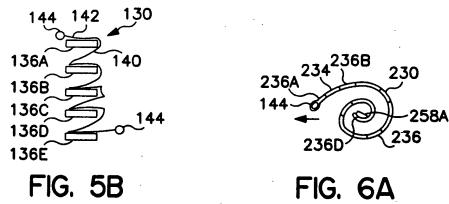


FIG. 4C








FIG. 6B

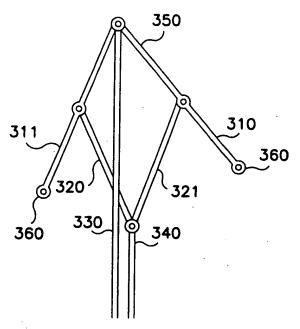


FIG. 7

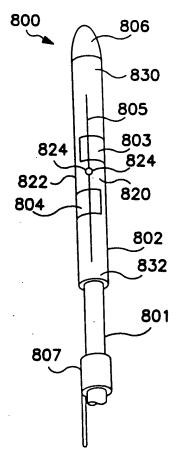
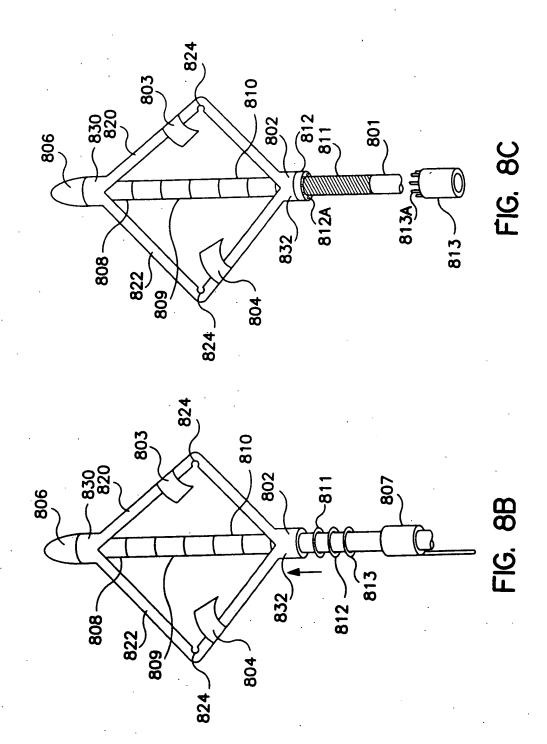
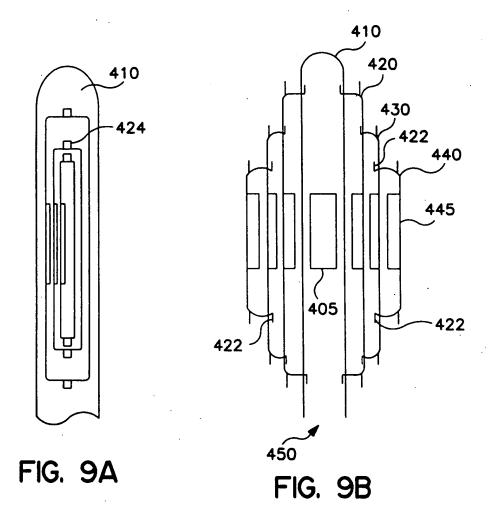


FIG. 8A





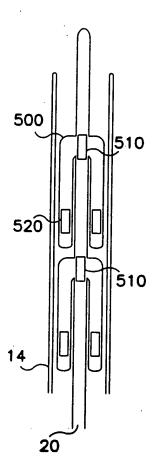


FIG. IOA

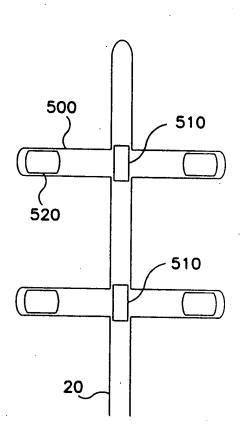


FIG. IOB

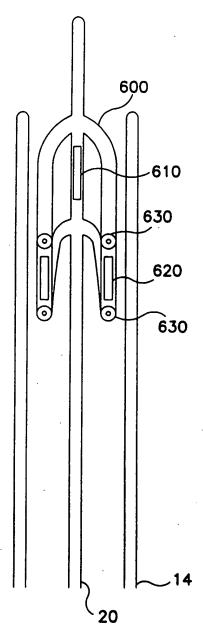


FIG. I IA

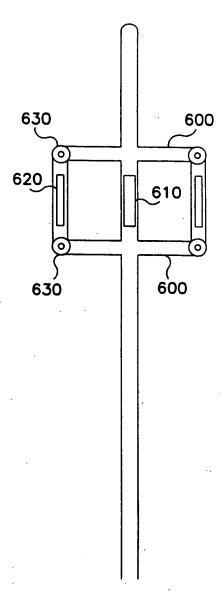
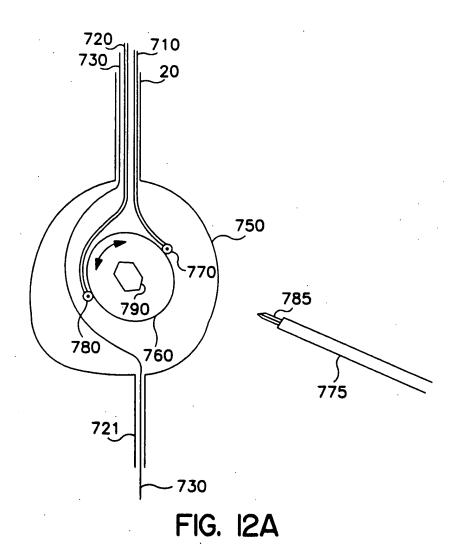


FIG. I IB



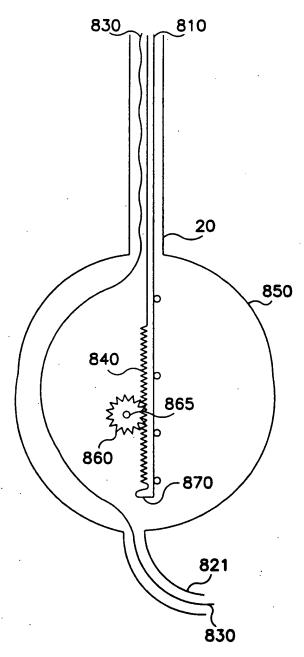


FIG. 12B

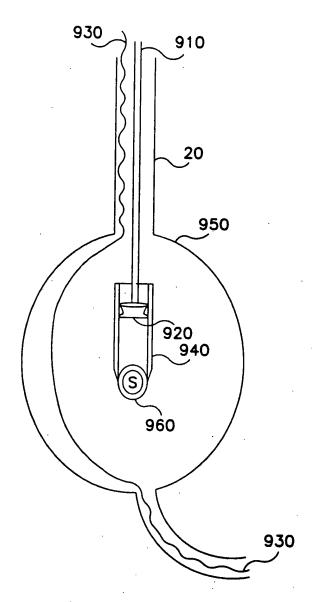


FIG. 12C

Banner & Witcoff, Ltd
Title: Apparatus and Method for Expanding A Stimulation Lead Body in Situ
Inventor: King et al.
Serial No.; (TBA)
Atty. Docket No. 11738.00215
Replacement Sheet Page 15 of 15

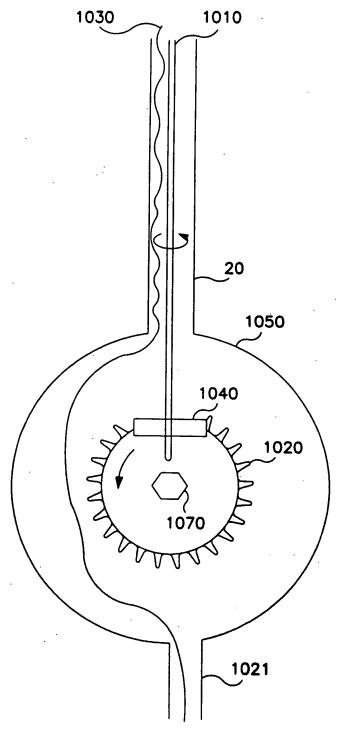


FIG. I2D